

AUGMENTED COMANIPULATION IN ROBOTIC SURGERY

B. Cagneau, D. Bellot, G. Morel,

*Institut des Systèmes Intelligents et Robotique, 18 route du Panorama, 92265 Fontenay Aux Roses, France
{cagneau,bellot,morel}@robot.jussieu.fr*

N. Zemiti

*TIMC-IMAG Laboratory, 38706 La Tronche Cedex France
nabil.zemiti@imag.fr*

G. D'Agostino

*Università Federico II di Napoli, Facoltà di Ingegneria dell'Automazione, Corso Umberto I, 80138 Napoli, Italy
gianluca82@gmail.com*

Keywords: Force control, robotic surgery, cobotic, augmented comanipulation.

Abstract: This paper presents a control scheme for augmented comanipulation with force feedback in robotic surgery. This approach aims at increasing the surgeon's dexterity. The surgeon manipulates a handle mounted on the robot which manipulates the instrument. The control law ensures that the instrument applies on the organ the same forces that the surgeon applies on the handle but decreased by a scale factor. As a consequence, the robotic device provides the surgeon with an augmented sensation of the interaction forces between the instrument and the organ. The proposed control law does not require any knowledge of the environment. This control scheme is proven stable thanks to a passivity study. Indeed, passivity analysis is a useful tool for the stability analysis of a robot interacting with an unknown environment. Experimental results are presented on a robot dedicated to minimally invasive surgery.

1 INTRODUCTION

In the context of robotic surgery, the surgeon and the medical staff have to interact with the robot. Depending on the surgical task, the degree of cooperation can be really different. Simple tasks may be realized by the robot, in an autonomous way, under the surgeon's supervision. For example, the surgeon defines the desired positions via an interface and the robot moves to these positions. However more complex tasks require the surgeon's judgment and, thus, cannot be performed autonomously by the robot. These tasks require that the robot works in cooperation with the surgeon. The surgeon's skills are thus improved as the robot increases his dexterity. To do so, one of the possibilities is robot's force control. For instance, in minimally invasive surgery, a robotic device could be used in order to display manipulation forces back to the surgeon. Indeed, since the instruments are manipulated through a trocar and because of the friction in the trocar, the surgeon loses the sensation of the interaction forces between the instrument and the organ

and his dexterity is thus reduced. An other application of force control that could increase the dexterity of the surgeon is force scaling. Indeed, for precise manipulation tasks, a robotic device could provide the surgeon with an augmented sensation of the interaction forces between the instrument and the organ. Comanipulation appears to be a good solution to overcome these problems. Comanipulation is a direct interaction between the surgeon and the robot: the instrument is manipulated simultaneously by the surgeon and by the robot. The main difference between comanipulation and teleoperation is that no master arm is needed to impose displacements to the robot. So the complexity and the cost of a comanipulation system may be lower since it involves only one mechanical system. Moreover, the use of a comanipulation system may be more intuitive for the human operator.

Different approaches have been studied concerning the comanipulation. Some systems are able to impose virtual constraints to the surgeon's gesture which restrain the tool into a delimited area of the task-space

and forbid the access to critical zones.

For example, in (Schneider et al., 2000), the system *PADyC* has been presented. The clinical results obtained with this system concern pericardial puncture. It consists to remove pathological liquid from the pericardium using a needle. *PADyC* can be used under different control modes corresponding to the degree of autonomy the surgeon wants. The robot is controlled with a velocity loop and it imposes constraints on the surgeon to prevent damages on the surface of the heart. These constraints are computed with respect to the relative position between the needle and the percutaneous access. Indeed, a model of the operation's area is created during a pre-operative phase. This model is then used to derive the constraints field. Here no force control is used to perform the operation.

In (Jakopec et al., 2003), the *Acrobot* system is used to assist the surgeon during an operation of knee replacement. The main feature of this system is to impose virtual constraints on the surgeon when he/she cooperates with the robot. When the task has been defined with the planning software, the manipulator is able to move freely the robot to the operations area. If the surgeon moves the tool outside the defined path, the robot applies forces on the user to modify the current trajectory. It has been clinically proven that the preparation of bones surfaces are more accurate comparing to a classical operation. Once again, no force control is performed with this system.

Moreover, some systems can exploit a measure of forces. Therefore, there is no need to use models of contacts to obtain the measure of distal forces. It is also possible to derive constraints which are directly based on the forces applied by the surgeon on the organs.

In (Kazanides et al., 1992), a force controller is used so that the surgeon can guide the robot. The surgical tool is attached below a force sensor mounted on the robot's wrist. The force controller uses the measured forces to provide the reference to an inner velocity control loop. When the desired force is null, any applied force on the instrument causes the robot to move in the direction of this force. So, the surgeon can guide the robot by holding the tool.

In the same manner, the *Surgicobot* system (Kochan, 2004) allows the surgeon and the robot to manipulate the same drilling instrument for maxillo-facial interventions. The surgeon can freely move the instrument except in some predefined space where the robot generates restrictive forces in order to prevent the surgeon from moving the instrument too close to vital nerves.

In (Taylor et al., 1999), (Kumar et al., 2000) and (Roy et al., 2002) augmented comanipulation ap-

proaches are presented: the surgeon holds a handle mounted on the robot and the robot manipulates the instrument in a way such as it exerts on the organ the same force that the surgeon applies on the handle, but scaled-down. Three different control laws using an inner position/velocity control loop are compared in (Roy et al., 2002). The best results are obtained with an adaptive control law involving the estimation of the environment's compliance. However, when the contact with the environment is lost, the estimation becomes problematic. Another disadvantage of this control law is that it requires differentiation of the force applied by the surgeon on the handle which is a noisy signal.

Even if benefits presented in the above references are important (e.g. gesture's accuracy or the increase of system's safety), none of these systems allow the surgeon to feel an amplified version of the distal forces acting between the tool and the organ.

In this paper, we present a control scheme for augmented comanipulation with force feedback. The main advantages of this control law is that it does not require any knowledge of the environment nor differentiation of a noisy signal. This approach is an extension of previous works (Zemiti et al., 2006) realized in our laboratory.

The first part of this paper is devoted to the proposed control law for augmented comanipulation. This control scheme is proven stable thanks to a passivity study in the second part. Experimental results with a robot dedicated to minimally invasive surgery are presented in the last part.

2 AUGMENTED COMANIPULATION

2.1 Principle of the Approach

We present, hereafter, a robotic device in order to assist the surgeon for accurate manipulation tasks requiring human judgment and involving small interaction forces between the surgical tool and the organ. Therefore, the proposed device allows an augmented comanipulation. It is a comanipulation system because the surgical instrument is held simultaneously both by the surgeon and by the robot. We call it augmented because the robot is controlled in such a way that the surgeon is provided with an amplified sensation of the interaction forces between the instrument and the organ. As a consequence, the instrument applies on the organ the same forces that the surgeon would apply in a transparent mode but decreased by a

scale factor. This device can also filter the surgeon's tremor in order to increase the accuracy of the task. This approach supposes that the reference forces provided by the surgeon and the interaction forces between the instrument and the organ may be measured separately. Therefore a handle equipped with a force sensor (force sensor 2) is mounted on the instrument (see figure 1). The surgeon manipulates this handle and the force sensor 2 measures the forces applied by the surgeon on the instrument at point O_2 . The force sensor 1 measures the forces applied by the organ on the instrument at point O_1 . The data provided

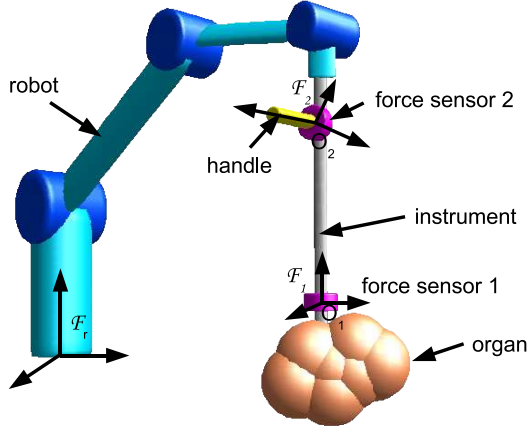


Figure 1: Setup for augmented comanipulation.

by the force sensor number i are wrenches applied on point O_i and expressed in the basis of frame \mathcal{F}_i linked to the sensor. In order to be compared these wrenches have to be expressed in the same point and in the same basis. As the transformations between the basis linked to frames \mathcal{F}_i and the basis linked to the fixed robot base frame \mathcal{F}_r are supposed to be known, we choose to express the wrenches in the basis linked to the frame \mathcal{F}_r . So, from the data provided by the force sensor 1, we can compute $-w_e$ the wrench applied by the organ on the instrument at point O_1 and expressed in frame \mathcal{F}_r . From the data provided by the force sensor 2, we can compute $-w_s$ the wrench applied by the surgeon on the instrument at point O_2 and expressed in frame \mathcal{F}_r . Note that w_e and w_s are respectively the wrench applied by the instrument on the organ at point O_1 and the wrench applied by the instrument on the surgeon at point O_2 . Assuming that the transformation between the frame \mathcal{F}_1 and the frame \mathcal{F}_2 is known, we can compute the wrench $-w_u$ applied by the surgeon on the instrument at point O_1 in \mathcal{F}_r : $-w_u = \mathbf{T}_{12}(-w_s)$ with

$$\mathbf{T}_{12} = \begin{bmatrix} \mathbf{I}_3 & \mathbf{0}_3 \\ -[O_2O_1]_{\times} & \mathbf{I}_3 \end{bmatrix}$$

where $[O_2O_1]_{\times}$ denotes the skew symmetric matrix associated with the vector from O_2 to O_1 expressed in the basis of frame \mathcal{F}_r . However, in future work, it will be interesting to compute this transformation with a calibration process. In the Section 4, we assume that the mechanical design is precise enough to have a good estimation of this transformation.

With these notations, as detailed in subsection 2.3, the aim of the proposed approach is to control the robot such that $w_u = -\frac{1}{\beta}w_e$ where $\beta \in]0; 1]$ i.e. the surgeon feels the forces applied by the organ on the instrument, $-w_e$, amplified by a scale factor $\frac{1}{\beta} > 1$. The proposed control scheme is presented in the following subsection.

2.2 Proposed Control Scheme

The robot dynamics is modeled by the general form:

$$\mathbf{M}(q)\ddot{q} + C(q, \dot{q})\dot{q} + \Gamma_v\dot{q} + G_g(q) = \tau - \tau_e - \tau_u \quad (1)$$

where $q \in \mathbb{R}^n$ denotes the joint positions, $\mathbf{M}(q)$ is the positive definite symmetric inertia matrix, $C(q, \dot{q})\dot{q}$ is a vector grouping the Coriolis and centrifugal joint torques, $\Gamma_v\dot{q}$ is a vector grouping the dissipative joint torques, $G_g(q)$ is a vector grouping the gravity joint torques, τ is the command vector for joint torques. $-\tau_e$ and $-\tau_u$ are the joint torques corresponding respectively to $-w_e$ and $-w_u$ i.e. $-\tau_e = \mathbf{J}^t(q)(-w_e)$ and $-\tau_u = \mathbf{J}^t(q)(-w_u)$ where $\mathbf{J}(q)$ is the Jacobian matrix of the robot at point O_1 , expressed in the basis of \mathcal{F}_r .

At the lowest level of the controller, a proportional velocity feedback is used in order to partially linearize the robot dynamics:

$$\tau = -\mathbf{B}\dot{q} + \widehat{G}_g(q) + \widehat{C}(q, \dot{q})\dot{q} + \tau_c \quad (2)$$

where \mathbf{B} is a symmetric positive definite matrix of feedback gains, τ_c is the new command vector for the joint torques, $\widehat{G}_g(q)$ and $\widehat{C}(q, \dot{q})\dot{q}$ are estimated values of $G_g(q)$ and $C(q, \dot{q})\dot{q}$. Therefore, the model (1) becomes:

$$\mathbf{M}(q)\ddot{q} + \mathbf{B}\dot{q} = \tau_c - \tau_e - \tau_u \quad (3)$$

The proposed control scheme is presented on figure 2.

In this figure the Jacobian matrix $\mathbf{J}(q)$ is noted \mathbf{J} . This control scheme introduces notations defined as follow:

- $C_{\tau}(s)$ is a Proportional-Integral torque compensator at the joint level such that:

$$C_{\tau}(s) = \mathbf{K}_p + \frac{\mathbf{K}_i}{s} \quad (4)$$

where $\mathbf{K}_p \in \mathbb{R}^{n \times n}$ and $\mathbf{K}_i \in \mathbb{R}^{n \times n}$ are symmetric, positive definite matrices.

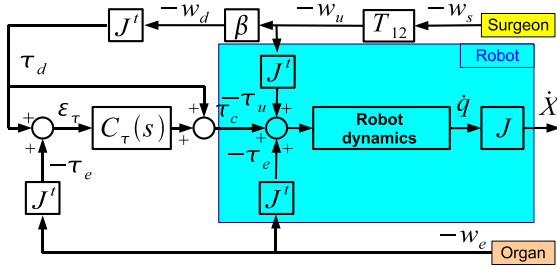


Figure 2: Augmented Comanipulation force control scheme in joint space.

- \dot{X} is the 6-component vector grouping the coordinates of the rotational and linear velocity of the instrument at point O_1 with respect to frame \mathcal{F}_r , expressed in the basis of \mathcal{F}_r .

In the sequel the following assumption will be used :

Assumption 1 *The matrix $\mathbf{J}(q)$ is of full rank n*

This assumption means that the robot is not in a singular configuration.

2.3 Equilibrium

The stability of the control scheme 2 will be proved in the following section. So, assuming that this control scheme is stable, as the controller $C_\tau(s)$ involves an integral term, the torque error ϵ_τ will be null at the equilibrium. So, at the equilibrium:

$$\tau_d - \tau_e = 0 \quad (5)$$

As the stable low-pass filter $G(s)$ has a steady-state gain equal to 1, at the equilibrium, $\tau_d = \mathbf{J}(q)^t \beta (-w_u)$. Thus (5) leads to :

$$\mathbf{J}(q)^t \left((-w_u) + \frac{1}{\beta} (-w_e) \right) = 0 \quad (6)$$

If $n = 6$ i.e. if we consider a 6 joints robot, the matrix $\mathbf{J}(q)$ is square. Moreover, according to assumption (1), this matrix is of full rank. Therefore, it can be deduced from equation (6) that:

$$w_u = \frac{1}{\beta} (-w_e) \quad (7)$$

Suppose that we choose $\beta = 1$. Then, equation (7) can be written:

$$w_u = (-w_e) \quad (8)$$

It means the wrench w_s sensed by the surgeon at point O_2 is such that its expression at point O_1 , w_u , is equal to the wrench $-w_e$ applied by the organ on the instrument expressed at point O_1 . Thus the surgeon

manipulates the instrument in a transparent way i.e. the surgeon senses the wrench w_s as if he/she were manipulating a zero mass instrument without any friction.

Similarly, if $\beta \in]0; 1[$, equation (7) means that the wrench w_s sensed by the surgeon is an amplified version, by the scale factor $\frac{1}{\beta} > 1$, of the wrench that he would sense in a transparent manipulation. Let's remark that (7) can be written $w_e = \beta (-w_u)$. It means that the wrench applied by the instrument on the organ at point O_1 is the wrench applied by the surgeon at the same point, reduced by the scale factor β .

If $n < 6$, $\mathbf{J}^t(q) \in \mathbb{R}^{n \times 6}$ is not square. Thus it cannot be deduced from (6) that the wrench error $\epsilon_w = (-w_u) + \frac{1}{\beta} (-w_e)$ is zero. The wrench error ϵ_w is not necessarily zero but belongs to the null space of $\mathbf{J}^t(q)$. An equilibrium is obtained between w_u and $\frac{1}{\beta} (-w_e)$.

3 PASSIVITY

In the proposed approach, the robot interacts with its environment. The stability of the control loop depends not only on the robot dynamics but also on the environment dynamics. However we cannot assume for a known model for the environment. Therefore, a useful tool for the stability analysis of the proposed control loop is passivity analysis since this study does not require any environments model. Thus, whatever could be the contacts (robot-organ / robot-surgeon), the passivity analysis ensures that the system remains stable. The principle of a passivity study is presented in the following subsection

3.1 Principle

Let consider an LTI system with an input u , an output y , such that $y = \mathbf{T}(s)u$ with $\mathbf{T}(s)$ a real rational transfer matrix. This system is passive if and only if $\mathbf{T}(s)$ is positive real. In turn, positive realness can be checked by the following property (Anderson and Vongpanitlerd, 1973):

Property 1 *Let $s_k = \sigma_k + j\omega_k$, $k \in \{1..m\}$, denote the m poles of all the elements $T_{ij}(s)$ of $\mathbf{T}(s)$, and let $j\omega_l$, $l \in \{1..p\}$, denote the $p \leq m$ pure imaginary poles of all the elements $T_{ij}(s)$ of $\mathbf{T}(s)$. The transfer $\mathbf{T}(s)$ is Positive Real if, and only if:*

1. $\forall k \in \{1..m\}, \sigma_k < 0$;
2. $\forall l \in \{1..p\}$, $j\omega_l$ is of multiplicity 1, and the associated residue matrix \mathbf{K}_l is hermitian, positive

semidefinite (PSD). The matrix \mathbf{K}_l can be computed as:

$$\mathbf{K}_l = \lim_{s \rightarrow j\omega_l} (s - j\omega_l) \mathbf{T}(s), \text{ if } \omega_l \text{ is finite}$$

and: $\mathbf{K}_l = \lim_{s \rightarrow \infty} \frac{\mathbf{T}(s)}{s}, \text{ if } \omega_l \text{ is infinite}$

Note that a zero of $T_{ij}(s)$ is considered as a pole at the infinity.

3. $\mathbf{T}'(-j\omega) + \mathbf{T}(j\omega) = \mathbf{T}^*(j\omega) + \mathbf{T}(j\omega)$ is PSD, for any $\omega \in \mathbb{R} - \{\omega_l, l \in \{1..p\}\}$. ■

Let, now, consider an LTI system with two different inputs u_1 and u_2 provided by two different environments, and assume that this system is described by: $y = \mathbf{T}_1(s)u_1 + \mathbf{T}_2(s)u_2$. This system is passive if and only if $\mathbf{T}_1(s)$ is positive real and $\mathbf{T}_2(s)$ is positive real.

3.2 Passivity of the Modified Force Control Scheme

3.2.1 Modeling, Linearized Robot Dynamics

The robot controlled by the control scheme depicted on figure 2 is a system whose output is \dot{X} . This system has two inputs $-w_u$ and $-w_e$ provided by two different environments, respectively the surgeon and the organ. So, in order to study the passivity of this system we first have to compute the transfer matrix $\mathbf{Y}_u(s)$ between $-w_u$ and \dot{X} and the transfer matrix $\mathbf{Y}_e(s)$ between $-w_e$ and \dot{X} . This computation supposes that the system is linear. Therefore, in order to study the passivity of the proposed control scheme, we linearize the robot dynamics (3) by assuming that the robot evolves in a neighborhood of a given joint configuration q_0 so that we can set $\mathbf{M} = \mathbf{M}(q_0)$ constant. The resulting linearized model writes:

$$\dot{q} = \mathbf{Y}_r(s)(\tau_c - \tau_u - \tau_e) \quad \text{with} \quad \mathbf{Y}_r(s) = (\mathbf{M}s + \mathbf{B})^{-1} \quad (9)$$

where s is the Laplace complex variable. Moreover, under the assumption that the robot evolves in a neighborhood of a given joint configuration q_0 , we can set $\mathbf{J} = \mathbf{J}(q_0)$ constant. Then, we get the following model:

$$\dot{X} = \mathbf{Y}_u(s)(-w_u) + \mathbf{Y}_e(s)(-w_e) \quad (10)$$

where:

$$\begin{cases} \mathbf{Y}_u(s) &= \mathbf{J}\mathbf{Y}_r(s) [\mathbf{I}_n + \beta(\mathbf{C}_\tau(s) + \mathbf{I}_n)] \mathbf{J}^t \\ \mathbf{Y}_e(s) &= \mathbf{J}\mathbf{Y}_r(s) [\mathbf{I}_n + \mathbf{C}_\tau(s)] \mathbf{J}^t \end{cases}$$

3.2.2 Passivity Study

The system (10) is passive if and only if the matrices $\mathbf{Y}_u(s)$ and $\mathbf{Y}_e(s)$ are positive real. As \mathbf{J} is supposed to be of full rank (Assumption 1), this condition is equivalent to the positive realness of the matrices $\mathbf{Y}_{u,2}$ and $\mathbf{Y}_{e,2}$ defined as follow:

$$\begin{cases} \mathbf{Y}_{u,2} &= \mathbf{Y}_r(s) [\mathbf{I}_n + \beta(\mathbf{C}_\tau(s) + \mathbf{I}_n)] \\ \mathbf{Y}_{e,2} &= \mathbf{Y}_r(s) [\mathbf{I}_n + \mathbf{C}_\tau(s)] \end{cases} \quad (11)$$

Equations (11), (9), and (4) lead to :

$$\begin{cases} \mathbf{Y}_{u,2} &= (\mathbf{M}s + \mathbf{B})^{-1} \left[\mathbf{I}_n + \beta\mathbf{K}'_p + \frac{\beta\mathbf{K}_i}{s} \right] \\ \mathbf{Y}_{e,2} &= (\mathbf{M}s + \mathbf{B})^{-1} \left[\mathbf{I}_n + \mathbf{K}_p + \frac{\mathbf{K}_i}{s} \right] \end{cases} \quad (12)$$

where $\mathbf{K}'_p = \mathbf{K}_p + \mathbf{I}_n$.

We first derive conditions ensuring the positive realness of $\mathbf{Y}_{u,2}(s)$. The poles of $\mathbf{Y}_{u,2}(s)$ are $s_1 = 0$ and the poles of $\mathbf{Y}_r(s)$. The poles associated to $\mathbf{Y}_r(s)$ are the solutions of $\det(\mathbf{M}s + \mathbf{B}) = 0$ i.e. the eigenvalues of $-\mathbf{M}^{-1}\mathbf{B}$. As far as \mathbf{M} and \mathbf{B} are symmetric positive definite matrices, the eigenvalues of $-\mathbf{M}^{-1}\mathbf{B}$ are negative real.

In order to check the second condition of property 1, we compute the residue \mathbf{K}_1 associated to pole $s_1 = 0$. We get:

$$\mathbf{K}_1 = \lim_{s \rightarrow s_1} s \mathbf{Y}_{u,2} = \beta \mathbf{B}^{-1} \mathbf{K}_i$$

As $\beta > 0$, we deduce the following condition for the passivity of the control scheme:

$$\mathbf{B}^{-1} \mathbf{K}_i \geq 0 \quad (13)$$

The third condition of property 1 consists in checking, for any $\omega \in \mathbb{R} - \{0\}$, the positive semidefiniteness of the matrix $\mathbf{H}_1(j\omega)$ defined as follow:

$$\begin{aligned} \mathbf{H}_1(j\omega) &= \mathbf{Y}_{u,2}(j\omega) + \mathbf{Y}_{u,2}'(-j\omega) \\ &= (j\omega\mathbf{M} + \mathbf{B})^{-1} \left[\mathbf{I}_n + \beta\mathbf{K}'_p + \frac{\beta\mathbf{K}_i}{j\omega} \right] \\ &\quad + \left[\mathbf{I}_n + \beta\mathbf{K}'_p + \frac{\beta\mathbf{K}_i}{-j\omega} \right] (-j\omega\mathbf{M} + \mathbf{B})^{-1} \end{aligned} \quad (14)$$

because \mathbf{K}'_p , \mathbf{K}_i , \mathbf{M} and \mathbf{B} are symmetric.

Positive semidefiniteness of $\mathbf{H}_1(j\omega)$ is equivalent to positive semidefiniteness of $\mathbf{H}_2(j\omega)$ defined as follow:

$$\begin{aligned} \mathbf{H}_2(j\omega) &= \frac{1}{\beta}(j\omega\mathbf{M} + \mathbf{B})\mathbf{H}_1(j\omega)(-j\omega\mathbf{M} + \mathbf{B}) \\ &= \left[\frac{1}{\beta}\mathbf{I}_n + \mathbf{K}'_p + \frac{\mathbf{K}_i}{j\omega} \right] (-j\omega\mathbf{M} + \mathbf{B}) \\ &\quad + (j\omega\mathbf{M} + \mathbf{B}) \left[\frac{1}{\beta}\mathbf{I}_n + \mathbf{K}'_p + \frac{\mathbf{K}_i}{-j\omega} \right] \end{aligned} \quad (15)$$

We get:

$$\mathbf{H}_2(j\omega) = \mathbf{R}_1 + \mathbf{R}_2 + j\omega\mathbf{Im}_1 + \frac{j}{\omega}\mathbf{Im}_2 \quad (16)$$

where:

$$\begin{aligned}\mathbf{R}_1 &= (2/\beta)\mathbf{B} \\ \mathbf{R}_2 &= \mathbf{K}'_p\mathbf{B} + \mathbf{B}\mathbf{K}'_p - (\mathbf{K}_i\mathbf{M} + \mathbf{M}\mathbf{K}_i) \\ \mathbf{Im}_1 &= \mathbf{M}\mathbf{K}'_p - \mathbf{K}'_p\mathbf{M} \\ \mathbf{Im}_2 &= \mathbf{K}_i\mathbf{B} - \mathbf{B}\mathbf{K}_i\end{aligned}$$

The hermitian matrix $\mathbf{H}_2(j\omega)$ must be PSD in order to ensure passivity. Thus its real part has to be PSD and its imaginary part has to be null. Therefore, the following conditions have to be satisfied for any $\omega \in \mathbb{R} - \{0\}$:

$$\mathbf{R}_1 + \mathbf{R}_2 \geq 0 \quad (17)$$

$$\omega\mathbf{Im}_1 + \frac{1}{\omega}\mathbf{Im}_2 = 0 \quad (18)$$

Thus, condition (18) is equivalent to:

$$\begin{cases} \mathbf{R}_1 + \mathbf{R}_2 \geq 0 \\ \mathbf{Im}_1 = 0 \\ \mathbf{Im}_2 = 0 \end{cases} \quad (19)$$

To summarize, the matrix $\mathbf{Y}_{u,2}(s)$ and thus $\mathbf{Y}_u(s)$ is positive real if and only if the following conditions are satisfied:

$$\begin{cases} \mathbf{B}^{-1}\mathbf{K}_i \geq 0 \\ \mathbf{Im}_1 = 0 \\ \mathbf{Im}_2 = 0 \\ \mathbf{R}_1 + \mathbf{R}_2 \geq 0 \end{cases} \quad (20)$$

As far as positive realness of $\mathbf{Y}_{e,2}(s)$ is concerned, with a similar reasoning we deduce that the first and the second condition of property 1 are satisfied if and only if $\mathbf{M}^{-1}\mathbf{B} > 0$ and $\mathbf{B}^{-1}\mathbf{K}_i \geq 0$. It can be noticed in equations (12) that the expression of $\mathbf{Y}_{e,2}(s)$ is similar to the expression of $\mathbf{Y}_{u,2}(s)$ when $\beta = 1$ and \mathbf{K}'_p is replaced by \mathbf{K}_p . Therefore, we deduce from equations (19) and (17) that the third condition ensuring the positive realness of $\mathbf{Y}_{e,2}(s)$ is satisfied if and only if:

$$\begin{cases} \mathbf{M}\mathbf{K}_p - \mathbf{K}_p\mathbf{M} = 0 \\ \mathbf{K}_i\mathbf{B} - \mathbf{B}\mathbf{K}_i = 0 \\ \mathbf{B} + \mathbf{K}_p\mathbf{B} - \mathbf{K}_i\mathbf{M} \geq 0 \end{cases} \quad (21)$$

The equations (20) and (21) lead to the following conditions for the passivity of the proposed control scheme:

$$\begin{cases} \mathbf{B}^{-1}\mathbf{K}_i \geq 0 \\ \mathbf{M}\mathbf{K}_p - \mathbf{K}_p\mathbf{M} = 0 \\ \mathbf{K}_i\mathbf{B} - \mathbf{B}\mathbf{K}_i = 0 \\ (\frac{1}{\beta}\mathbf{I}_n + \mathbf{K}'_p)\mathbf{B} - \mathbf{K}_i\mathbf{M} \geq 0 \end{cases} \quad (22)$$

with $\mathbf{K}'_p = \mathbf{K}_p + \mathbf{I}_n$.

4 EXPERIMENTS

The aim of these experiments is to show that it is possible to provide force feedback to the surgeon thanks to proposed control scheme. Furthermore, for different values of the gain β , we will verify that the system remains stable. Experimental setup will be briefly described and benefits of augmented comanipulation will be evaluated experimentally.

Note that, in the rest of the paper, the used joint torque compensator gains and the values of \mathbf{B} and β were chosen in such a way that the conditions given in 22 are verified.

4.1 Experimental Setup

The robot MC^2E (French acronym for *compact manipulator for endoscopic surgery*) is a Kinematically Defective Manipulator (KDM) which means that it has fewer joints than the dimension of the space in which its end-effector evolves. It is specially suited for minimally invasive robotic surgery applications (Zemiti et al., 2007). With $n = 4$ joints and a spherical structure, this robot provides 4 degrees of freedom (DOFs) at the instrument tip.

The Figure 3 shows how the mechanical constraint

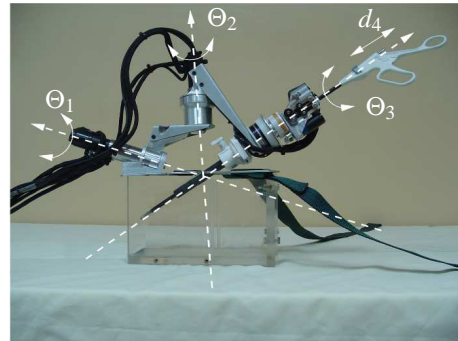


Figure 3: MC^2E can comanipulate an instrument with a surgeon, and measures wrenches that are applied either by the surgeon, or at the instrument tip.

is created. The lower part of the robot is dedicated to the orientation of the instruments. The upper part allows translation and rotation of the instrument along its own axis.

Since the 4 axis coincide, there is a fulcrum point which allows the insertion of the trocar into the patient's body. This mechanical structure is clearly adapted to Mini Invasive Surgery. Traumatismes are reduced because translations through the fulcrum point are not allowed.

Apart from its compactness, the main feature of this robot is that it offers a possibility for force

measurement in MIS. Namely, MC^2E can measure the distal organ-instrument interaction with a 6-axis force-torque sensor placed outside the patient. Thus, it is subject to much less sterilization constraints. Remarkably, due to the special mounting of the force sensor, these measurements are not affected by the disturbance forces and torques arising from the interaction between the trocar and the instrument.

It is important to mention that the control scheme that we have detailed in Section 2 can be used in other fields of interest and not only in laparoscopic surgery. For example, it is possible to improve surgeon accuracy during otologic surgery. The forces applied during such kinds of interventions are very low. Therefore, it should be useful to provide an amplified version of these forces thanks to force feedback.

The new control scheme presented in section 2 indicates that the robot interacts with two different environments (the organ and the surgeon). This configura-

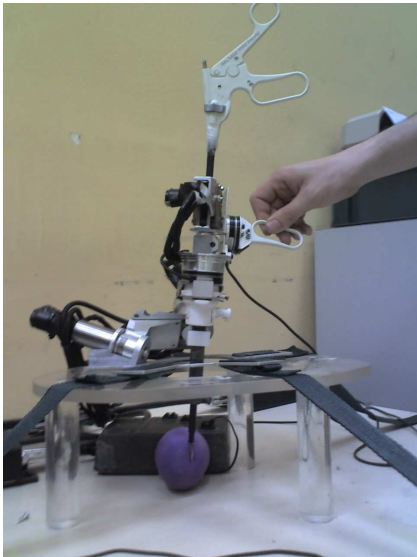


Figure 4: Experimental Setup.

tion is shown on figure 4. It needs a second force sensor to measure forces between the robot and the surgeon. Therefore to measure forces applied by the surgeon, a second force sensor has been added on the robot. Due to difficulties to fix it directly on the handle, it has been deported on the second axis of MC^2E . This particular disposition was the quickest way to provide force feedback to the manipulator. However, the same disposition is not adapted to transmit forces along instrument's axis. In order to overcome this problem, next step will be to modify existing experimental setup to exploit each of the robot's DOF.

4.2 Experimental Results

The figure 5 shows how the gain β has been modified during the experiment. $\beta = 1$ is a particular value

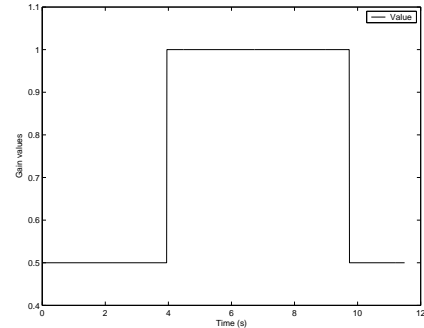


Figure 5: Gain values vs. time.

for which torques measured on the organ are equal to torques applied by the manipulator. When setting $\beta = 0.5$, torques applied on the organ should be decreased by a factor 2.

The figure 6 depicts torque measurements. It allows to compare torques applied on the organ, torques provided to the controller and torques applied on the manipulator. This result demonstrates that the proposed

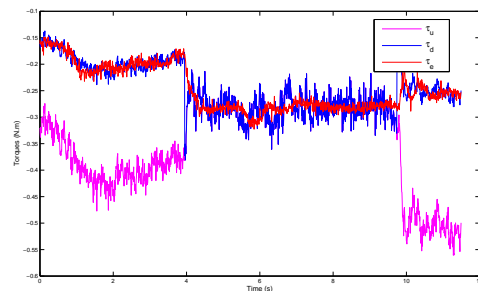


Figure 6: Torque values vs. time.

control scheme allows a reduction of the torques applied on the organ. At $t = 10s$, β is switched from 1.0 to 0.5. One can notify that torques applied on the organ almost remain the same but torques applied by the surgeon are amplified. Therefore, to apply the same efforts on the organ, the surgeon must amplify forces acting on the robot. This result satisfies equation (7). The figure 7 shows that the system remains stable for different values of gains. Furthermore, it demonstrates that good performances can be achieved with the controller which has been proposed in section 2. Error appearing on Figure 7 is mainly due to noise on measurement. However, one can notice that there are some error peaks on this plot. This phenomenon is due to the modification of the force feedback gain

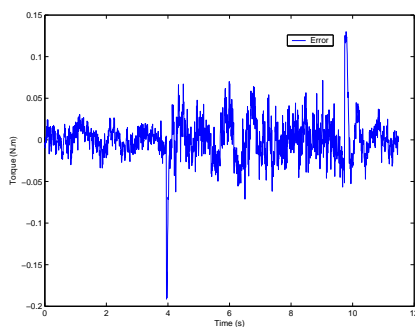


Figure 7: Torque error vs. time.

during experiments. In practice, if a fixed value of β is used, these peaks would not appear.

5 CONCLUSIONS

This paper presents a modified version of a force control scheme. In the context of comanipulation, it is possible to provide force feedback to the manipulator by modifying torques reference. In order to obtain such results, a second force sensor is necessary to distinguish manipulator and environment forces.

Robots kinematic has been used to deal with torques equilibrium. In other words, using a gains matrix allows reduction of forces acting on the environment and amplification of forces acting on the manipulator. Experiments have been conducted to show efficiency of the proposed control scheme.

Moreover, a formal proof of passivity has been established. It ensures stability of the system whatever could be contacts between the robot and its environment.

In future work, in-vivo experiments will be conducted. Even if experiments are satisfying with actual experimental setup, it should be modified to exploit the last 2 DOFS. A new handle seems to be the easiest way to use existing robot.

ACKNOWLEDGEMENTS

Barthélemy Cagneau would like to acknowledge Clara Lord for her contribution to this work. Scientific and technical discussions have been very useful to improve the quality of this paper.

REFERENCES

- Anderson, B. D. and Vongpanitlerd, S. (1973). *Network Analysis and Synthesis - A Modern Systems Theory Approach*. Englewood Cliffs, N.J. , Prentice-Hall.
- Jakopec, M., Baena, F., Harris, S., Gomes, P., Cobb, J., and Davies, B. (2003). The hands-on orthopaedic robot acrobot: Early clinical trials of total knee replacement surgery. *IEEE Transactions on Robotics and Automation*, 19(5):902–911.
- Kazanzides, P., Zuhars, J., Mittelstadt, B., and Taylor, R. H. (1992). Force sensing and control for a surgical robot. In *Proceedings of the IEEE International Conference on Robotics and Automation*, pages 612–617.
- Kochan, A. (2004). A cobotic solution for surgical applications. *Industrial Robot: An International Journal*, 31:478–480.
- Kumar, R., Berkelman, P., Gupta, P., Barnes, A., Jensen, P. S., Whitcomb, L. L., and Taylor, R. H. (2000). Preliminary experiments in cooperative human/robot force control for robot assisted microsurgical manipulation. In *Proceedings of the IEEE International Conference on Robotics and Automation*, pages 610–617.
- Roy, J., Rothbaum, D. L., and Whitcomb, L. L. (2002). Haptic feedback augmentation through position based adaptive force scaling: theory and experiment. In *Proceedings of the IEEE/RSJ International Conference on Intelligent Robots and Systems*, pages 2911–2919.
- Schneider, O., Troccaz, J., Chavanon, O., and Blin, D. (2000). Padyc: a synergistic robot for cardiac puncturing. In *Proceedings of the IEEE International Conference on Robotics and Automation*, pages 2883–2888.
- Taylor, R., Jensen, P., Whitcomb, L., Barnes, A., Kumar, R., Stoianovici, D., Gupta, P., Wang, Z., deJuan, E., and Kavoussi, L. (1999). A steady-hand robotic system for microsurgical augmentation. *International journal of robotics research*, 18:1201–1210.
- Zemiti, N., Morel, G., Micaelli, A., Cagneau, B., and Bellet, D. (2006). A passive formulation of force control for kinematically constrained manipulators. In *Proceedings of the IEEE International Conference on Robotics and Automation*, pages 2238–2243.
- Zemiti, N., Morel, G., Ortmaier, T., and Bonnet, N. (2007). Mechatronic design of a new robot for force control in minimally invasive surgery. *IEEE/ASME Transactions on Mechatronics*, 12(2):143–153.