

On the design of ergonomic wearable robotic devices for motion assistance and rehabilitation

Azzurra Chiri, Marco Cempini, *Student Member, IEEE*, Stefano Marco Maria De Rossi, *Student Member, IEEE*, Tommaso Lenzi, *Student Member, IEEE*, Francesco Giovacchini, Nicola Vitiello, *Member, IEEE*, and Maria Chiara Carrozza *Member, IEEE*

Abstract— The appropriate ergonomic design of a wearable robotic device is critical for the effectiveness of the device itself.

In this paper we identified two key requirements for a structural ergonomics: the correct kinematic compatibility with the human limb and a comfortable and adaptable physical human-robot interface. We then show how the aforementioned requirements have been faced and implemented in the mechanical design of two wearable devices for elbow and hand rehabilitation, both developed at The BioRobotics Institute of Scuola Superiore Sant' Anna.

I. INTRODUCTION

TO fulfill the requirements for an *ergonomic* design of a wearable robotic system for motion assistance and rehabilitation, the physical interaction between the human users and the elements of the system should be carefully taken into account. In particular, the ergonomic design of wearable robotic devices that are, by definition, parallel and physically coupled with a human limb should be compliant with the human model in terms of anatomical, anthropometric and biomechanical characteristics [1].

In the last decades a multitude of wearable interfaces for upper or lower limbs were proposed for rehabilitation or assistance of disabled people (e.g. [2],[3]). However, a critical analysis of the current state-of-the-art evidences that little attention has been paid in the appropriate ergonomic design of the majority of current wearable interfaces [4].

For a successful ergonomic design two main aspects need to be considered: the actuation/control and the mechanical/kinematic design of the structure.

In this paper we will only focus on the second point, since while most researchers are concentrating their work on improving the first aspect, the second issue is less investigated even if equally important. Indeed while sophisticated interaction control laws and variable impedance actuators can fulfill the requirements for providing the desired assistive and rehabilitation strategies [5],[6], the physical-human-robot interface (pHRI) of most of current wearable interfaces, does not always allow an

effective *kinematic coupling* with the user limb and a comfortable force interaction.

Both *kinematic compatibility* and *comfortable mechanical physical-interface* are essential requirements for ergonomics, and if one only of these two requirements fails, wearable robots lose their effectiveness and final end-user acceptability is affected. On one hand, if the kinematics setting of a wearable device is not correctly matched to the patient limb, undesired interaction forces can be generated during the motion of the device. Such joint-axes misalignment can then cause undesired translational forces on human articulations that, in the worst scenario, can lead to an uncomfortable or even painful use of the device [7]. On the other hand, instead, the specific choice of the mechanical interface influences the physical interaction with the user, so determining the perceived comfort and effort experienced by subjects [4]. These aspects become even more important if the final users are unhealthy subjects.

Rather, all types of wearable robots must be safe, comfortable and able to smoothly interact with human users.

The goal of this paper is then to review and discuss the main design criteria for truly ergonomic mechanical design of wearable interfaces for assistance/rehabilitation. Furthermore, how these criteria have been fulfilled in the design of two wearable devices developed at the Scuola Superiore Sant'Anna is following shown.

II. CRUCIAL ASPECTS IN ERGONOMICS

An ergonomic system is able to provide a gentle and comfortable interaction with the human subject, by exploiting the full range of motion (ROM) of the human limb within its maximum natural workspace.

From a practical point of view this can be fulfilled *a)* if the system ensures the correct *kinematic compatibility* with the human limb and *b)* if the mechanical structure provides a *comfortable* and *adaptable* human-robot interface. Each single aspect will be analyzed in the following, by presenting two case studies of wearable devices for assistance and rehabilitation (i.e. NEUROExos [8],[9] and HANDEXOS [10],[11]), entirely designed at The BioRobotics Institute of the Scuola Superiore Sant' Anna and conceived to match the main requirements for a truly ergonomic design.

A. Kinematic compatibility

A key requirement for the pHRI of an ergonomic wearable robot is the correct and auto-adjustable alignment between the device and the patient's kinematic rotational axes. This is

This work was supported in part by the European WAY project (FP7- ICT-2011-288551), the European CYBERLEGs project (FP7-ICT-2011-CYBERLEGS), the national AMULOS project (Industria 2015, MI01 00319) and the regional EARLYREHAB project (Regione Toscana, Health Regional Research Programme 2009). Authors are with The BioRobotics Institute, Scuola Superiore di Studi Universitari e di Perfezionamento Sant'Anna, viale Rinaldo Piaggio, 34, 56025, Pontedera, Pisa, Italy. Azzurra Chiri is corresponding author to provide phone: +39 050 883472, fax: +39 050 883497, e-mail: a.chiri@sssup.it.

difficult to achieve for several reasons: firstly, the exact location of the human rotational axes cannot be easily identified because of its inner position in the limb. Secondly, biological joints are not hinge joints. Rather, they have complex joint surface geometries due to bones morphology which can cause little translation of joints centre of rotation and change of rotational-axis orientation along with the joint motion (i.e. human joints are loose hinge joints). Thirdly, fixation of a robotic device on a human limb is never rigid, but slippage between the device and the limb will occur because of tissue deformations. Additionally, inter-subject and intra-subject variability make difficult the adaptation to different users with variable anthropometry.

All these reasons are likely to create human-robot axes misalignment so that torques applied to the robotic joint would generate reaction forces on the correspondent human articulation. Such forces, if not compensated, can finally lead the exoskeleton to become ineffective or even be painful/dangerous for the user. Risk of injury and discomfort has been proved if the kinematic mismatch between the wearable orthosis and the user are not correctly compensated [12]. Furthermore, it has been shown that such kinematic mismatch can also alter the correct muscular activation patterns during physical therapy, so leading to possible injury [13].

Another common cause of kinematic misalignment between wearable robots and the human articulation arises from oversimplification of the human joint kinematics. For example, common mistakes are to model the human shoulder joint as a “ball and socket type” joint, or again the hand metacarpo-phalangeal (MCP) articulation as simple ‘hinge’ joint.

– *Case-study 1: NEUROExos*

Despite its apparent simplicity, the elbow joint behaves as a loose hinge joint because of its intrinsic laxity. Its peculiarity, indeed, is that the flexion-extension rotational axis traces the surface of a double quasi-conic frustum with an elliptical cross-section [14] notably dependent on inter- and intra-subjects variability.

NEUROExos is a powered elbow exoskeleton with double-shell links (Fig. 1). It has been conceived in order to provide an active assistance of the flexion/extension elbow motion, but also to have a passive compliance with the laxity of the human elbow articulation. This choice allowed for a truly kinematic compatibility with the user’s articulation within its natural ROM.


From a mechanical point of view, such kinematic compliance has been provided by mounting the active rotational joint of the NEUROExos with a 4-degree of freedom (DOF) passive mechanism. It consists of 4 prismatic, 4 spherical, 2 circular sliders, 2 universal and 1 rotational joint [8]. These passive DOFs allow the flexion/extension rotational axis of the exoskeleton to rotate in the frontal plane of $\pm 15^\circ$, in the horizontal

plane of $\pm 21^\circ$ and to translate in the horizontal plane along the antero-posterior direction of ± 15 mm.


Moreover, the NEUROExos forearm link can slide along the flexion/extension axis of ± 15 mm. Lastly, the user’s upper arm can slide against the NEUROExos upper shell through ad-hoc elastic bushings, so to unload the elbow articulation from any frontal-plane component of the misalignment translational force.

There is no evidence in literature of wearable devices that can provide such level of compliance towards the user’s limb kinematics.

On the contrary, there are examples of robotic orthosis that restrict limb’s movements by reducing the number of DOFs through which the user is allowed to move. This is the case of the Lokomat gait orthosis. In this case legs movements is restricted to the sagittal plane without possibility of hip rotation or legs abduction/adduction. Therefore Lokomat training imposes an adaptation of the users gait to a modified pattern and consequently to a different muscular activation.

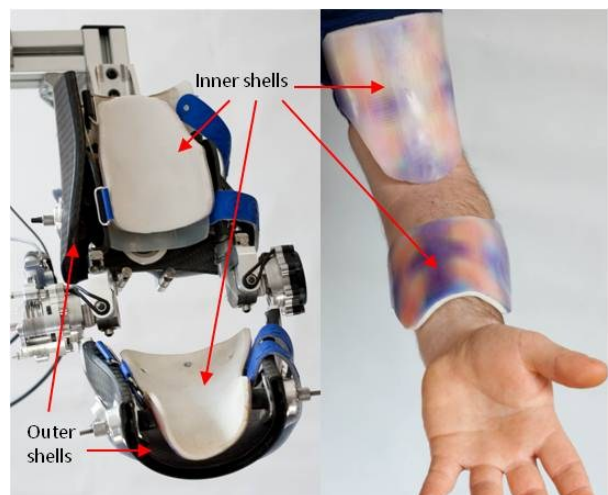

(a)

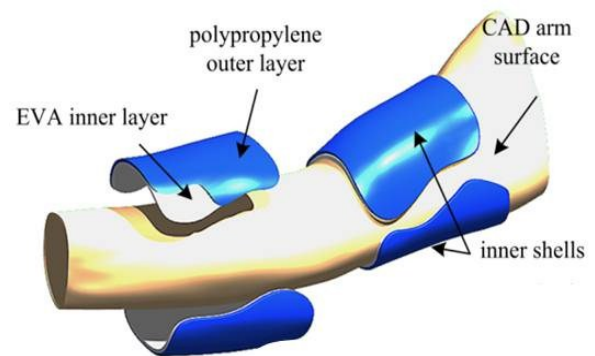

(b)

Fig. 1. Panel a): Overview of the NEUROExos shelled structure; panel b): detail of the inner shells, adaptable to the user’s limb morphology.

– *Case-study 2: HANDEXOS*

Also the mechanical design of HANDEXOS, a powered hand exoskeleton, has been focused on the requirement of a kinematic coupling between the user's and the exoskeleton joints.

The full compliance with the complex anatomy of the human hand is difficult to be achieved and nowadays represents one of the major challenges in robotics. Focusing on the HANDEXOS index finger module, it has been conceived in order to be compliant with the flexion/extension motion of each joint: MCP, proximal-interphalangeal (PIP) and distal-interphalangeal (DIP) joints.

However not all the hand articulations have the same anatomy: the PIP and DIP joints are hinge joints, with the head of the phalanx pulley-shaped with only one transverse axis; the MCP joint is an ellipsoidal joint that moves about two axes. In particular, during flexion the plate of the phalanx moves past the metacarpal head that has a variable radius of curvature [14]. This implies a variable relative distance between MCP and PIP joints.

So the MCP articulation is the most difficult to be assisted with a wearable hand device for the complexity of its anatomy that leads the center of rotation not to be fixed during finger flexion/extension. Moreover, differently from the other finger joints, its inner position in the palm does not allow to directly place a pulley on the joint's rotational axis.

From a mechanical point of view, the HANDEXOS PIP and DIP joints were implemented via revolute DOFs aligned along the PIP and DIP axes (Fig. 2), and equipped with an idle pulley for the actuation cable routing. In order to comply with their negligible misalignment, a soft cover in Neoprene was placed at the finger-exoskeleton interface in order to absorb potential axes misalignment.

For the correct kinematic compatibility with the entire user's finger, a self-aligning architecture [11] was developed for the MCP joint. It consists of a parallel chain made of two revolute and one linear DOFs (Fig. 2). This solution allowed to decouple joint rotation from joint translation [7], so allowing the transfer of the desired torque to the flexion/extension axis, without painful misalignment forces and maintaining low the overall size of the system.

On the contrary, usually the need for joint alignment imposes additional and complex regulations along the kinematic chain that, in the specific case of hand exoskeletons, leads to bulky mechanical solutions as, for example, in the case of the Wege's hand exoskeleton [15].

B. Comfort and adaptability

Other fundamental requirements for an ergonomic wearable device are the comfort of the structure and its adaptability to users anthropometry.

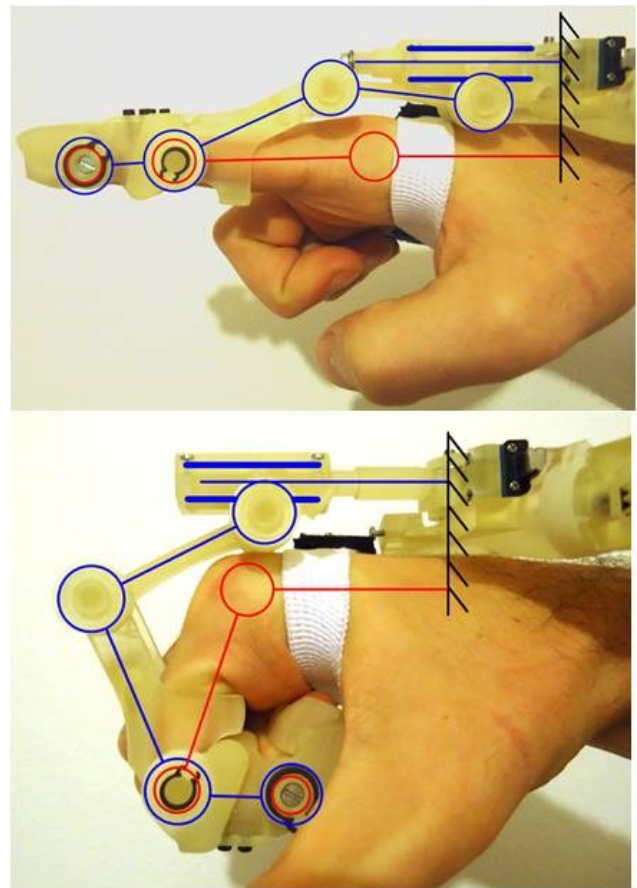


Fig. 2. Overview of the HANDEXOS finger module and kinematic layout in the extended (top) and flexed (bottom) configuration.

A truly comfortable device should have a lightweight mechanism and a wide distributed human-robot interface that does not cause discomfort or safety hazards during motion. Usually, in wearable devices the driving power is transmitted by means of connection band-cuff, while an increased contact surface can reduce the interaction pressure and thus the deriving stress/sore on the user limb.

Adaptability, instead, specifically refers to the possibility to fit different shape/size of the coupled human limb. If the anthropometric data (i.e. limb length and joints ROM) are not taken into account during the design of a wearable system, the device becomes unusable or even dangerous for the user.

Even if comfort and adaptability requirements are highly interrelated, an ergonomic design requires the individual accomplishment of each of them.

– *Case-study 1: NEUROExos*

The NEUROExos links have been designed as a double-shelled structure composed of two concentric shells, namely inner and outer shells (Fig. 1a). The inner shells are then composed of two dorsal and two ventral shells, appositely designed on the morphology of the human limb (Fig. 1b)

Such a mechanical solution allows to overpass the common limitations of the typical bar-shaped links of

most of the exoskeletons presented in literature (i.e. slippage of the connecting cuffs and non-distributed fixation pressure on the human limb, with consequent skin sore and discomfort). Rather, the shells shape ensures a gentle transfer of loads thanks to a wide interaction area and simplify the donning-on procedure. The latter being fundamental if users are non-collaborative patients.

The two carbon-fiber NEUROExos outer shells provide structural stiffness to the exoskeleton, and transfer the assistive load to the human upper arm and forearm.

The two NEUROExos inner shells are passive orthoses made of orthopaedic material, in contact with the dorsal and ventral sides of the user's limb segment (Fig. 1b). In order to enhance the ergonomic adaptability to the user's limb of each individual subject, the two inner shells can be thermo-shaped on a plaster cast of the user's limb. In this way it is possible to achieve a perfectly adaptable contact-area. Alternatively, standard sizes of shells can be manufactured in order to fit most of the users anthropometry.

This solution is preferable to the usual belts fastened to the user's limb since shells increase the contact area, thus reducing the interaction pressure and the localized stress. Instead, in the case of the LOKOMAT leg orthosis, the fact that the system has been carefully thought in order to be adaptable to individual users, by keeping variable the alignment with the patients' hip, knee, and ankle joints, it does not guarantee a comfortable usage of the system. On the contrary, skin sores and stumbling of the patient were reported, due to the slippage of the orthosis cuffs during the training session.

– Case-study 2: HANDEXOS

Similarly to the NEUROExos case, also HANDEXOS has been designed with a shelled structure in order to allow a distributed contact-area with the finger's skin.

In particular, each phalangeal link has a C-shaped shell structure, appositely designed in order to both reduce the lateral encumbrance between two close finger modules, and to only burden the external lateral side of each finger. Such solution, also simplify the donning-on/donning-off procedure.

Furthermore, the compliance with the requirement of the adaptability has been fulfilled by endowing HANDEXOS with specific solutions for fitting the inter-subject anthropometric variability. In particular, the self-aligning MCP mechanism can absorb variations in dimensions of the first finger phalanx. The distal exoskeleton phalanx, instead, has been appositely designed with an untapped distal end, while the middle phalanx has an adjustable dovetail coupling, which can be adapted to the user's phalanx length.

III. CONCLUSION

A truly ergonomic wearable device smoothly interacts with the user's limb and provides a safe and comfort human-robot interface. In this paper we identified two main key-requirements for a structural ergonomics: the correct kinematic axes alignment with the human limb and a comfortable and adaptable pHRI.

Each single aspect has been then analyzed with two examples of practical implementation of the aforementioned requirements, starting from the analysis of the biological case to the definition of the appropriate mechanical solutions.

REFERENCES

- [1] A.M. Dollar, H. Herr, "Lower Extremity Exoskeletons and Active Orthoses: Challenges and State-of-the-Art", *IEEE Transactions on Robotics*, vol. 24, pp. 144-158, 2008.
- [2] A. Frisoli, F. Salsedo, M. Bergamasco, B. Rossi, and M.C. Carboncini, "A force-feedback exoskeleton for upper-limb rehabilitation in virtual reality", *Applied Bionics and Biomechanics*, 1754-2103, vol. 6(2), pp. 115-126, 2009.
- [3] M. Iwaki, Y. Hasegawa, and Y. Sankai, "Fingertip stiffness control using antagonistic pairs of polyarticular tendons drive system," in *Proc. IEEE Int. Conf. Robot. Biomimetics*, Guilin, China, 2009, pp. 925-930.
- [4] A. Schiele and F.C. van der Helm, "Kinematic Design to Improve Ergonomics in Human Machine Interaction", *IEEE Transaction on Neural Systems and Rehabilitation Engineering*, vol. 14(4), pp. 456-469, 2006.
- [5] Z. Jia-Fan, Y. Can-Jun, C. Ying, Z. Yu, D. Yi-Ming, "Modeling and control of a curved pneumatic muscle actuator for wearable elbow exoskeleton", *Mechatronics*, vol. 18, pp. 448-457, 2008.
- [6] K. Kiguchi, T. Tanaka, and T. Fukuda, "Neuro-fuzzy control of a robotic exoskeleton with EMG signals", *IEEE Transactions on Fuzzy Systems*, vol. 12(4), pp. 481-490, 2004.
- [7] A.H.A. Stienen, E.E.G. Hekman, F.C.T. van der Helm, and H. van der Kooij, "Self-Aligning Exoskeleton Axes Trough Decoupling of Joint Rotations and Translations", *IEEE Transactions on Robotics*, vol. 25(3), pp. 628-633, 2009.
- [8] N. Vitiello, T. Lenzi, S. Roccella, S.M.M. De Rossi, E. Cattin, et al., "NEUROExos: a powered elbow exoskeleton designed for physical rehabilitation", *IEEE Trans. Robotics*, submitted for publication.
- [9] T. Lenzi, N. Vitiello, S.M.M. De Rossi, S. Roccella, F. Vecchi, M.C. Carrozza, "NEUROExos: a variable impedance powered elbow exoskeleton", *IEEE International Conference on Robotics and Automation*, 2011.
- [10] A. Chiri, N. Vitiello, F. Giovacchini, S. Roccella, F. Vecchi, and M.C. Carrozza, "Mechatronic design and characterization of the index finger module of a hand exoskeleton for post-stroke rehabilitation", *IEEE/ASME Trans. Mechatronics*, DOI: 10.1109/TMECH.2011.2144614.
- [11] M. Cempini, S.M.M. De Rossi, A. Chiri, T. Lenzi, F. Giovacchini, N. Vitiello, and M.C. Carrozza, "Kinematic and actuation design of a wearable hand exoskeleton for rehabilitation", *IEEE/RSJ International Conference on Intelligent Robots and Systems 2012*, submitted.
- [12] G. Colombo, M. Joerg, and V. Diez, "Driven gait orthosis to do locomotor training of paraplegic patients," presented at the 22nd Annu. EMBS Conf., Chicago, IL, Jul. 23-28, 2000.
- [13] J. M. Hidler and A. E. Wall, "Alterations in muscle activation patterns during robotic-assisted walking," *Clin. Biomech.*, vol. 20, pp. 184-193, 2005.
- [14] I.A. Kapandji, "Fisiologia articolare. Arto Superiore", Editions \ MALOINE, Paris, France, 2002.
- [15] A. Wege and G. Hommel, "Embedded system design for a hand exoskeleton," in *Embedded Systems—Modeling, Technology, and Applications*. Netherlands: Springer-Verlag, 2006.